

Dr. Name _____ Phone # _____


Acct. # _____ Patient Name _____
First Last

Address/Email _____ Deliver by 5 p.m. on See Reverse for Working Times

Enclosed with case: Impressions Models Bite Photos Other: _____

Rx


See reverse for supported
implant systems



All Restorations
Made in the USA

Signature _____ License # _____
(see reverse for limited warranty details)

Indicate System and Diameter

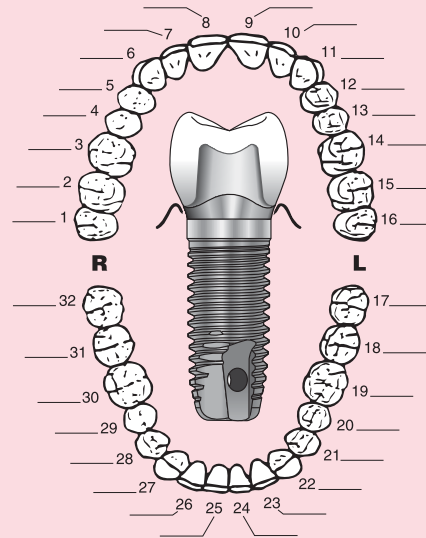

FINAL CERAMIC SHADE



Indicate Shade Here

OCCUSAL STAINING

Light* Med Dark None

PONTIC DESIGN




INCISAL SHAPE INSTRUCTIONS




Rounded Squared Pointed

MARGIN/METAL DESIGN

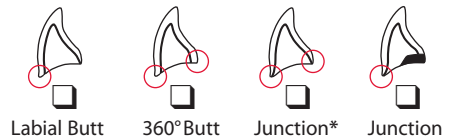

Labial Butt 360° Butt Junction* Junction

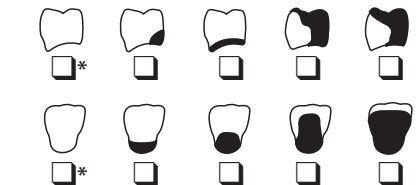

*Standard unless specified otherwise

Abutment Margin Design



Shoulder for
all-ceramic*

Chamfer for
PFM/BruxZir*

METAL-FREE

- BruxZir Solid Zirconia*
- IPS e.max CAD
- IPS e.max Press
- PrismaTik Clinical Zirconia
- Lava Crowns & Bridges

PFM & Full-Cast

- Non-Precious*
- Noble (semi-precious)
- Noble-Cast 45
- Noble-Cast 60*
- Noble-Cast 67
- White High Noble

BITE SPLINTS

- Upper Lower
- Comfort H/S (hard/soft)*
- Comfort (hard)
- Soft EVA Nightguard

CUSTOM IMPLANT ABUTMENTS

- Titanium
- All-Zirconia
- Screw-Retained BruxZir Crown w/ Ti-Base
- Zirconia w/ Ti-Base
- Prepare existing abutment

INCLUSIVE® CUSTOM TITANIUM AND ZIRCONIA W/TI-BASE ABUTMENTS ARE COMPATIBLE WITH THE FOLLOWING IMPLANT SYSTEMS

Biomet 3i [†] Certain [†]	Camlog [†] Screw-Line [†]	Dentsply Implants [†] Astra Tech Implant System [†]	Glidewell Direct [†] Inclusive® Tapered Implant System	Keystone Dental [†] PrimaConnex [†]
Neoss [†] Neoss [†]		Nobel Biocare [†] Brånemark System [†] NobelActive [†] NobelReplace [†]	Straumann [†] Bone Level [†]	Zimmer Dental [†] Screw-Vent [†]

INCLUSIVE® CUSTOM ALL-ZIRCONIA ABUTMENTS ARE COMPATIBLE WITH THE FOLLOWING IMPLANT SYSTEMS

Biomet 3i [†] Certain [†]	Glidewell Direct [†] Inclusive® Tapered Implant System	Nobel Biocare [†] NobelReplace [†]	Zimmer Dental [†] Screw-Vent [†]
--	---	---	---

INCLUSIVE® CAD/CAM MILLED IMPLANT BARS ARE COMPATIBLE WITH THE FOLLOWING IMPLANT SYSTEMS

Biomet 3i [†] Certain [†] External Hex [†] (4.1mm)	Camlog [†] Screw-Line [†]	Dentsply Implants [†] Astra Tech Implant System [†]	Glidewell Direct [†] Inclusive® Tapered Implant System	Keystone Dental [†] PrimaConnex [†]
Neoss [†] Neoss [†]		Nobel Biocare [†] Brånemark System [†] NobelActive [†] NobelReplace [†]	Straumann [†] Bone Level [†] synOcta [†] (RN/WN)	Zimmer Dental [†] Screw-Vent [†]

*# Not a trademark of Las Vegas Digital Dental Restorations.
Las Vegas Digital Dental Restorations works in partnership with Neoss and Keystone.
Inclusive is a registered trademark of PrismaDentalcraft Inc.*


TERMS AND WARRANTY INFORMATION

*Please allow full working time for each product selected. Working times are **NOT** guaranteed and do **NOT** include weekends or holidays. Only \$6 shipping per box **EACH** way (contiguous U.S. only; shipping charge varies for Alaska, Hawaii and Puerto Rico).
We honor **VISA, MASTERCARD, AMEX and DISCOVER.***


TERMS: Cost of collection of any account will be paid by the customer. All accounts are payable within 30 days of statement date. **Accounts not paid within the stated terms will be subject to COD status and a late charge of 2 percent of the unpaid balance.** Prices subject to change without notice.

LIMITED WARRANTY/LIMITATION OF LIABILITY. Las Vegas Digital Dental Solutions (“the lab”) warrants that all dental devices (a “device”) are made according to your specification and approval in the belief that the device will be useful and **MAKES NO OTHER WARRANTIES INCLUDING, BUT NOT LIMITED TO, ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.** Subject to the return of a device that is placed and then fails, the lab will repair or replace the device without charge for the cost of materials and workmanship or refund the original price paid, at the lab’s option, as follows: (1) screw-retained implant abutments up to 20 years (including replacement of a device that was made by the lab that was attached to said abutments and including an Inclusive® Tapered titanium dental implant upon request at no extra charge); (2) porcelain to metal, all ceramic (including screw-retained zirconia bridges), all metal, single-unit inlay, onlay and crown composite resin final prosthetics and milled implant bars, up to seven years; (3) composite resin bridges (excluding Maryland and inlay/onlay bridges) up to five years; (4) thermoformed appliances and splints if the failure is due to defects in materials or workmanship, provisionals, composite resin Maryland and inlay/onlay bridges, up to six months; (5) all other dental devices up to thirty days if the failure is due to defects in materials or workmanship. This Warranty is exclusively for your benefit, is not transferable and does not extend to any patients. You agree to pay all other costs of adjustment, repair and replacement of a device. Except where prohibited by law, the lab **WILL NOT BE LIABLE FOR ANY LOSS OR DAMAGES ARISING FROM THE USE OF A DEVICE, WHETHER DIRECT, INDIRECT, SPECIAL, INCIDENTAL OR CONSEQUENTIAL,** regardless of the theory asserted, including warranty, contract, negligence or strict liability and if such disclaimer is not permitted by law, the duration of any implied warranty is limited to 90 days from the date of delivery. In the event of a dispute and absent an amicable resolution the parties mutually agree to waive class actions in favor of mandatory individual arbitration of claims under this limited warranty in and in accordance with the laws of Nevada. The lab does not guarantee the performance of independent carriers.

CROWN PREPARATION GUIDELINES



- A. 2 mm incisal reduction
- B. 1.5 mm middle third reduction
- C. Labial and lingual walls must be convergent
- D. Preparation should be cut in three planes

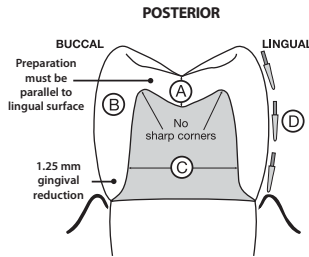

- A. 2 mm occlusal reduction
- B. 1.5 mm middle third reduction
- C. Buccal and lingual walls must be convergent
- D. Preparation should be cut in three planes

IN-LAB WORKING TIMES

Please allow full working time for each product selected. Working times are **NOT** guaranteed and do **NOT** include weekends or holidays.

CAD/CAM PFMs	5 working days
Full-Cast Restorations	5 working days
Metal-Free Restorations	5 working days
Custom Implant Abutments	5 working days
Restorations over Implants	5 working days
Bite Splints	4 working days

All rush cases must be prescheduled by calling **800-936-1848** before the case is shipped.
Time of pickup may affect turnaround time.

FOR LAB USE ONLY
TELEPHONE CALL RECORD

Dr. _____ Acct. # _____

Patient Name _____

RE: _____

Result _____

Date due in office _____

Date of call _____ Initials _____